#### ПІДТВЕРДЖУВАЛЬНЕ ПОВІДОМЛЕННЯ

Державне підприємство «Український науково-дослідний і навчальний центр проблем стандартизації, сертифікації та якості» (ДП «УкрНДНЦ»)

Наказ від 11.12.2018 № 475

ISO/IEC 11801-1:2017/Cor 1:2018

Information technology — Generic cabling for customer premises — Part 1: General requirements

прийнято як національний стандарт методом підтвердження за позначенням

ДСТУ ISO/IEC 11801-1:2018/Поправка № 1:2018 (ISO/IEC 11801-1:2017/Cor 1:2018, IDT)

Інформаційні технології. Кабельні системи загальної призначеності для приміщень користувачів. Частина 1. Загальні вимоги

3 наданням чинності від 2019-01-01

Відповідає офіційному тексту

#### ISO/IEC 11801-1

Edition 1.0 2017-11

## INFORMATION TECHNOLOGY – GENERIC CABLING FOR CUSTOMER PREMISES

Part 1: General requirements

#### CORRIGENDUM1

#### **Foreword**

Replace, in list item d), "Category BCT-B, 8.1, and 8.2;" with "Categories BCT-B, 8.1 and 8.2;".

Replace list item f) with the following new list item:

f) addition of cabled optical fibre Categories OS1a and OM5;

Replace, in list item g), "silica optical fibre cabling;" with "optical fibre classes;"

Replace list item h) with the following new list item:

h) cabled optical fibre Categories OM1, OM2 and OS1 have been moved to an informative annex.


#### Introduction

Replace the first paragraph with the following new paragraph:

This document contains general requirements in support of the other premises-specific referenced cabling design documents developed by ISO/IEC JTC 1/SC 25 including ISO/IEC 11801-2, ISO/IEC 11801-3, ISO/IEC 11801-4, ISO/IEC 11801-5, ISO/IEC 11801-6, related Technical Specifications and Technical Reports (including the ISO/IEC TR 11801-99xx series, ISO/IEC TR 24704, ISO/IEC TR 24750 and ISO/IEC TS 29125).

## Figure 1 – Relationships between the generic cabling documents produced by ISO/IEC JTC 1/SC 25

Replace the figure graphic with the following new figure graphic:

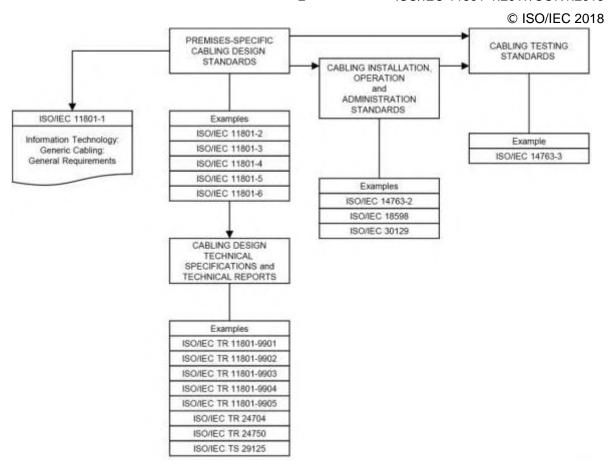

#### 3.1 Terms and definitions

In 3.1.26, delete "end-to-end" from the definition.

Delete the entire entry 3.1.32.

#### 3.2 Abbreviations

Insert the following abbreviation:

C connection

Replace:

FEXT far-end crosstalk attenuation (loss) with:

FEXT far-end crosstalk (loss) Replace:

NEXT near-end crosstalk attenuation (loss)

with:

NEXT near-end crosstalk (loss)

#### 3.3.1 Variables

Delete the following line:

C connection

#### 3.3.2 Indices

Delete the following line:

TO index to denominate a characteristic, measured from the TO


#### 5.1 Functional elements

After the sentence "Groups of these functional elements are connected together to form cabling subsystems.", insert the following new note:

NOTE The numbering of the cabling subsystems does not imply a hierarchy.

#### Figure 5 - Equipment and test interfaces

Replace the figure graphic with the following new figure graphic:

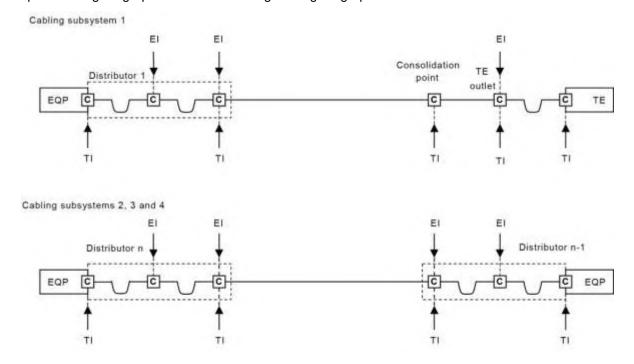

#### Table 2 - Details of environmental classification

In row 20, insert "g/m<sup>3</sup>" after each numerical value in columns 2, 3 and 4, as follows:

Sodium chloride (salt/sea water)	0 g/m <sup>3</sup>	< 0,3 g/m <sup>3</sup>	< 0,3 g/m <sup>3</sup>
----------------------------------	--------------------	------------------------	------------------------

#### In row 21, insert "mg/m<sup>3</sup>" after each numerical value in columns 2, 3 and 4, as follows:

, 3			
Oil (dry-air concentration)	0 mg/m <sup>3</sup>	< 0,005 mg/m <sup>3</sup>	< 0,5 mg/m <sup>3</sup>
(for oil types see b)			

## In row 22, insert "mg/m<sup>3</sup>" after each numerical value in columns 3 and 4, as follows:

Sodium stearate (soap)	None	> 5 × 10 <sup>4</sup> mg/m <sup>3</sup> aqueous non-gelling	> 5 × 10 <sup>4</sup> mg/m³ aqueous gelling

## In rows 26 to 35, insert "mg/m<sup>3</sup>" after each numerical value in columns 2, 3 and 4, as follows:

Hydrogen sulphide	< 0,003 mg/m³/ < 0,01 mg/m³	< 0,05 mg/m³/ < 0,5 mg/m³	< 10 mg/m <sup>3</sup> / < 50 mg/m <sup>3</sup>
Sulphur dioxide	< 0,01 mg/m³/ < 0,03 mg/m³	< 0,1 mg/m <sup>3</sup> / < 0,3 mg/m <sup>3</sup>	< 5 mg/m <sup>3</sup> / < 15 mg/m <sup>3</sup>
Sulphur trioxide (ffs)	< 0,01 mg/m³/ < 0,03 mg/m³	< 0,1 mg/m <sup>3</sup> / < 0,3 mg/m <sup>3</sup>	< 5 mg/m <sup>3</sup> / < 15 mg/m <sup>3</sup>
Chlorine wet (> 50 % humidity)	< 0,000 5 mg/m³/ < 0,001 mg/m³	< 0,005 mg/m³/ < 0,03 mg/m³	< 0,05 mg/m³/ < 0,3 mg/m³
Chlorine dry (< 50 % humidity)	< 0,002 mg/m³/ < 0,01 mg/m³	< 0,02 mg/m³/ < 0,1 mg/m³	< 0,2 mg/m <sup>3</sup> / < 1,0 mg/m <sup>3</sup>
Hydrogen chloride	-/<0,06 mg/m <sup>3</sup>	< 0,06 mg/m³/ < 0,3 mg/m³	< 0,6 mg/m <sup>3</sup> / 3,0 mg/m <sup>3</sup>
Hydrogen fluoride	< 0,001 mg/m³/ < 0,005 mg/m³	< 0,01 mg/m³/ < 0,05 mg/m³	< 0,1 mg/m <sup>3</sup> / < 1,0 mg/m <sup>3</sup>
Ammonia	< 1 mg/m <sup>3</sup> / < 5 mg/m <sup>3</sup>	< 10 mg/m <sup>3</sup> / < 50 mg/m <sup>3</sup>	< 50 mg/m <sup>3</sup> / < 250 mg/m <sup>3</sup>
Oxides of nitrogen	< 0,05 mg/m³/ < 0,1 mg/m³	< 0,5 mg/m <sup>3</sup> / < 1 mg/m <sup>3</sup>	< 5 mg/m <sup>3</sup> / < 10 mg/m <sup>3</sup>
Ozone	< 0,002 g/m <sup>3</sup> / < 0,005 g/m <sup>3</sup>	< 0,025 g/m <sup>3</sup> / < 0,05 g/m <sup>3</sup>	< 0,1 g/m³/ < 1 g/m³

#### 6.3.1 General

In the first sentence after list item 2), replace "two sub-Classes, L and M." with "two sub-Classes, L and M (see Table 5)."

#### 6.3.3.2 Insertion loss/attenuation

In the last paragraph before Table 5, delete ", at maximum implementation,".

#### 6.3.3.6 Direct current loop resistance

Replace the first paragraph with the following new paragraph:

The DC loop resistance requirements are applicable to all cabling Classes.

#### 6.3.3.7 Direct current resistance unbalance

Replace the first paragraph with the following new paragraph:

The DC resistance unbalance requirements are applicable to all cabling Classes.

#### 6.3.3.10 Propagation delay

Replace the first paragraph with the following new paragraph:

The propagation delay requirements are applicable to all cabling Classes.

#### **6.3.3.11 Delay skew**

Replace the first paragraph with the following new paragraph:

The delay skew requirements are applicable to all cabling Classes.

#### 6.3.3.12.2 Unbalance attenuation, near-end

In the second paragraph, first sentence, replace the two instances of the word "systems" with "channels".

#### Table 21 - TCL for channel for unscreened systems

In the title of Table 21, replace the word "systems" with "channels".

At the end of footnote b, add the following new text:

" $f_u$  is the upper frequency of the Class."

#### Table 25 – ELTCTL for channel for unscreened systems

In the title of Table 25, replace the word "systems" with "channels".

#### Table 29 – Coupling attenuation for a channel for screened systems


In the title of Table 29, replace the word "systems" with "channels".

#### 6.3.3.13.2 Power sum alien NEXT

In the second paragraph, delete ", at maximum implementation,".

#### Figure 7 - Link designations

Replace the figure graphic with the following new figure graphic:

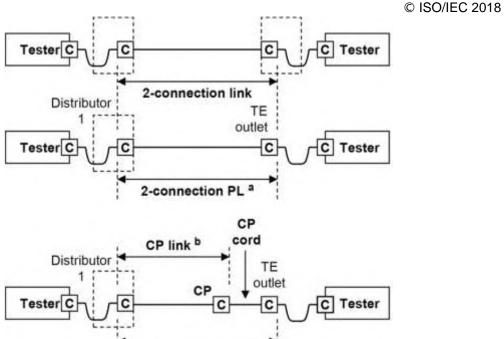

3-connection PL c

#### 7.2.1 General

In the last paragraph, delete the following sentence:

Link requirements for unbalance attenuation and coupling attenuation are ffs.

#### Table 84 - Backbone link length equations

Replace list item 1) with the following new list item:

1) 0,2 % per °C for screened balanced cables up to 60 °C,

# Figure 12 – Four position jack pin and pair grouping assignments for IEC 61076-2-101 connecting hardware (front view of connector)

Replace the Figure 12 title with the following new title:

# Figure 12 – Four position connector pin and pair assignments for IEC 61076-2-101 connecting hardware (front view of male connector)

# Figure 13 – Eight position jack pin and pair grouping assignments for IEC 61076-2-109 connecting hardware (front view of connector)

Replace the Figure 13 title with the following new title:

Figure 13 – Eight position connector pin and pair grouping assignments for IEC 610762-109 connecting hardware (front view of male connector)

#### Table 140 - Informative values of return loss for balanced cords at key frequencies

In the first column, delete "ffs" at frequency value 2 000.

#### Table E.1 – Applications using balanced cabling

In rows 25 and 26, replace, in the second column, "IEEE 802.3bz:2016" with "ISO/IEC/IEEE 8802-3:2017/AMD7", as follows:

Ethernet 2.5GBASE-T	ISO/IEC/IEEE 8802- 3:2017/AMD7, Clause 126 <sup>a</sup>	2016	2.5 Gigabit Ethernet over Twisted Pairs, IEEE 802.3bz
Ethernet 5GBASE-T	ISO/IEC/IEEE 8802- 3:2017/AMD7, Clause 126 <sup>a</sup>	2016	5 Gigabit Ethernet over Twisted Pairs, IEEE 802.3bz

In row 35, replace "20xx" with "2017", as follows:

#### Class I 2017 (defined up to 2000 MHz)

In rows 36 and 37, replace, in the second column, "IEEE 802.3bq:2016" with "ISO/IEC/IEEE 8802-3:2017/AMD3", as follows:

Ethernet 25GBASE-T	ISO/IEC/IEEE 8802- 3:2017/AMD3, Clause 113	2016	25 Gigabit Ethernet over Twisted Pairs, IEEE 802.3bq
Ethernet 40GBASE-T	ISO/IEC/IEEE 8802- 3:2017/AMD3, Clause 113	2016	40 Gigabit Ethernet over Twisted Pairs, IEEE 802.3bq

In row 38, replace "20xx" with "2017", as follows:

## Class II 2017 (defined up to 2000 MHz)

In rows 39 and 40, replace, in the second column, "IEEE 802.3bq:2016" with "ISO/IEC/IEEE 8802-3:2017/AMD3", as follows:

Ethernet 25GBASE-T	ISO/IEC/IEEE 8802- 3:2017/AMD3, Clause 113	2016	25 Gigabit Ethernet over Twisted Pairs, IEEE 802.3bq
Ethernet 40GBASE-T	ISO/IEC/IEEE 8802- 3:2017/AMD3, Clause 113	2016	40 Gigabit Ethernet over Twisted Pairs, IEEE 802.3bq

In the text box, in the first paragraph, replace two instances of "10GBase-T" with "10GBASE-T".

In the text box, in the second paragraph, replace two instances of "2.5GBase-T" with "2.5GBASE-T".

In the text box, in the fourth paragraph, first sentence, replace "are" with "is".

In the text box, in the fourth paragraph, second sentence, delete two instances of "(ffs)".